
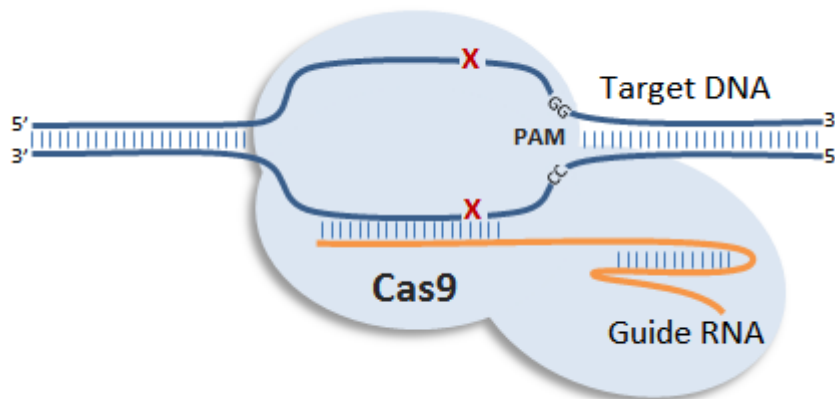



CHRND-R399H Genotyping Strategy

Animals have been engineered using the CRISPR/Cas9 technology. Most of the knockout alleles generated through this method will be obtained by deletion of a critical exon or by introduction of an indel (insertion/deletion) within the coding sequence of a critical exon (see picture below).

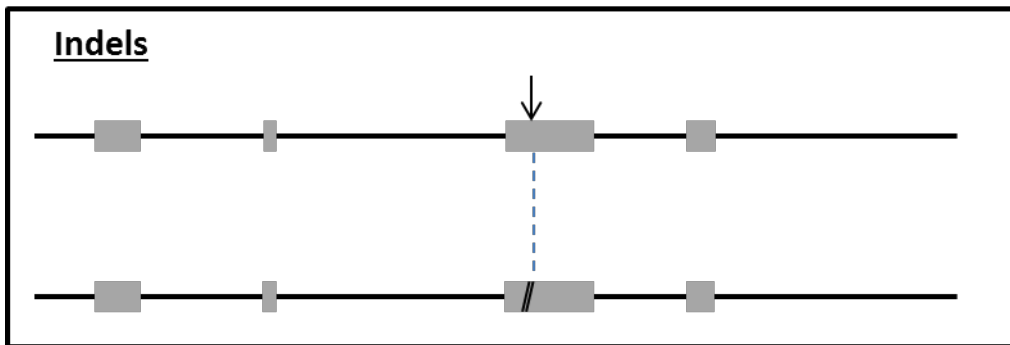


qPCR genotyping strategy

Standard PCR is the amplification of DNA between a pair of primers. Quantitative PCR employs the same principal as standard PCR, although it actually monitors the progress of the DNA synthesis as it occurs. The progress of the reaction is measured by using a Taqman probe. This is a short DNA oligo that is complimentary to part of the DNA sequence between the forward and reverse primers. At the 5' end of the probe there is a fluorescent reporter (R) and at the 3' end a quencher (Q). Whilst they are in close contact with each other there is no fluorescent signal.

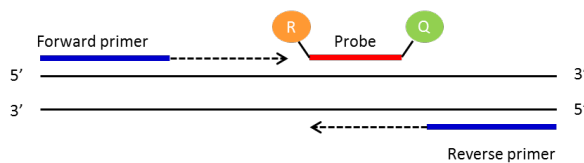

As the forward primer is extended the reporter is cleaved from the probe resulting in a fluorescent signal being detected. Once the primer extends enough to release the quencher this signal is blocked. By using probes with different fluorescent signals multiple PCR assays can be multiplexed and run together.

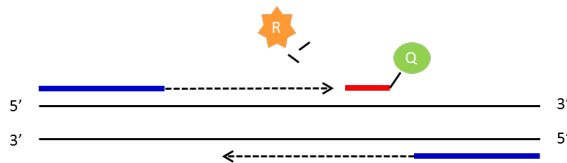

Allele specific primer and probe amplification assay (ASPPAA) PCR

This is a new real-time PCR method (Billard *et al.*, 2012) in which an allele specific primer and an allele specific probe designed specific to the SNPs. The primer is designed such a way that its 3' end ends with a specific SNP. The probe is also designed specific to the SNPs at its 3' end giving a primer probe overlap. A maximum of 3nt overlap between a primer and probe is allowed.


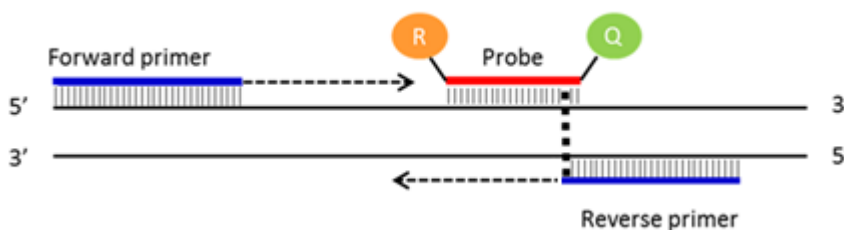


Figure1: Figure showing principle of ASPPAA PCR. The dotted line indicates the position of the SNP.

PCR reaction plot

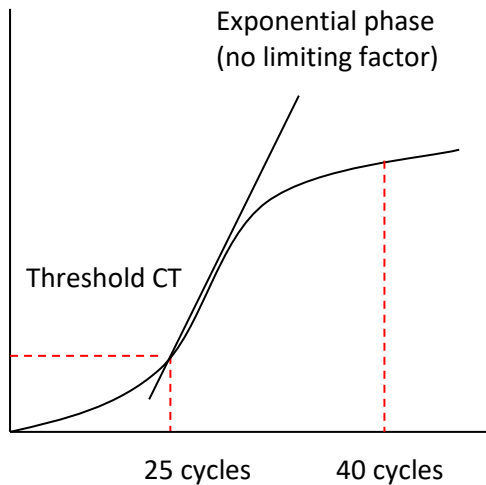

The number of cycles the PCR takes to reach a set threshold is known as the CT value. This is inversely correlated to the amount of template DNA in the sample.

e.g. CT 25 = 2 x template DNA
CT 26 = 1 x template DNA
CT above 30 = no template represented in the sample

CT value can be used to determine how many copies of a particular allele samples have.

All our qPCR are run in duplicate. A FAM labelled genotyping assay is run in multiplex with a VIC labelled internal control Dot1l.

References:

Billard A., Laval V., Fillinger S., Leroux P., Lachaise H., Beffa R., et al. (2012).
The allele-specific probe and primer amplification assay, a new real-time PCR method for fine quantification of single-nucleotide polymorphisms in pooled DNA.
Appl. Environ. Microbiol. 78 1063–1068. 10.1128/AEM.06957-11



CHRND-R399H Genotyping Strategy

Samples are genotyped with both WT and Mutant assays. These are FAM labelled assays that are designed to detect the critical exon that has been modified. If the animal contains the modified allele the copy number of the WT assay should drop by 1 and the mutant assay should raise by 1. For autosomal genes that have been targeted this means the following

- WT= 2 copies of the WT assay and 0 copies of the Mutant assay
- HET = 1 copy of the WT assay and 1 copy of the Mutant assay
- HOM = 0 copies of the WT assay and 2 copies of the Mutant assay

CHRND-R399H CRISPR/Cas9 mutant in which SNPs are as highlighted


WT ACTTAAGTCCG CAGTGACCTC
 Mutant ACTTAAGTACA CAGTGACCTC

CHRND-R399H-WT1 assay (FAM labelled probe)

GTCCCGCCAGCAGAGGAAGACCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATA
 CATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTCCCGCAGTGACCTCATGTTTGAGAAGCAATCA
 GAGCGGCATGGGCTGGCCCGGCCTCACCACAGCCCCTGAGTTCTGGTAGCCTTGGAACGTGGCC

CHRND-R399H-WT1 primers and probe

Primer 1 = CGCCAGCAGAGGAAGAC
 Primer 2 = CTCAAACATGAGGTCACTGCGG
 Probe = CCAGGGCTCTCATCCGGAGAAGC



CHRND-R399H-MUT1 assay (FAM labelled probe)

GTCCCGCCAGCAGAGGAAGACCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATA
 CATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTCCACAGTGACCTCATGTTTGAGAAGCAATCA
 GAGCGGCATGGGCTGGCCCGGCCTCACCACAGCCCCTGAGTTCTGGTAGCCTTGGAACGTGGCC

CHRND-R399H-MUT1 primers and probe

Primer 1 = CGCCAGCAGAGGAAGAC
 Primer 2 = CTTCTCAAACATGAGGTCACTGTGT
 Probe = CCAGGGCTCTCATCCGGAGAAGC

Dot1l internal control (VIC labelled)

CCCCTCTAGTCGTTTTCTGTTAGTAGTTGGCATCCTTATGCTTCATCTTACAGTCCGACTTGAGAGCTGGCCCTGA
 ATGGTCGTGCTGGGGCAAGGCTTTATTTTCAGGCGTAGCACACATGGTGGCCAATGGGACTCTGTAGGATCTGCCC


Primer 1 = GCCCCAGCACGACCATT
 Primer 2 = TAGTTGGCATCCTTATGCTTCATC
 Probe = CCAGCTCTCAAGTCG



qPCR master mix

ABI GTX Taqman master mix	5µl
Primers Dot1L_2F (20µM)	0.225µl
Primers Dot1L_R (20µM)	0.225µl
Probe DotL_2M (5µM)	0.2µl
FAM Assay (probe 5µM & primers 15µM each)	0.3µl
ddH2O	1.55µl
DNA (1/10 dilution of ABI Sample-to-SNP prep)	2.5µl

CHRND-R399H copy called result, image showing both replicates and controls (T250546)

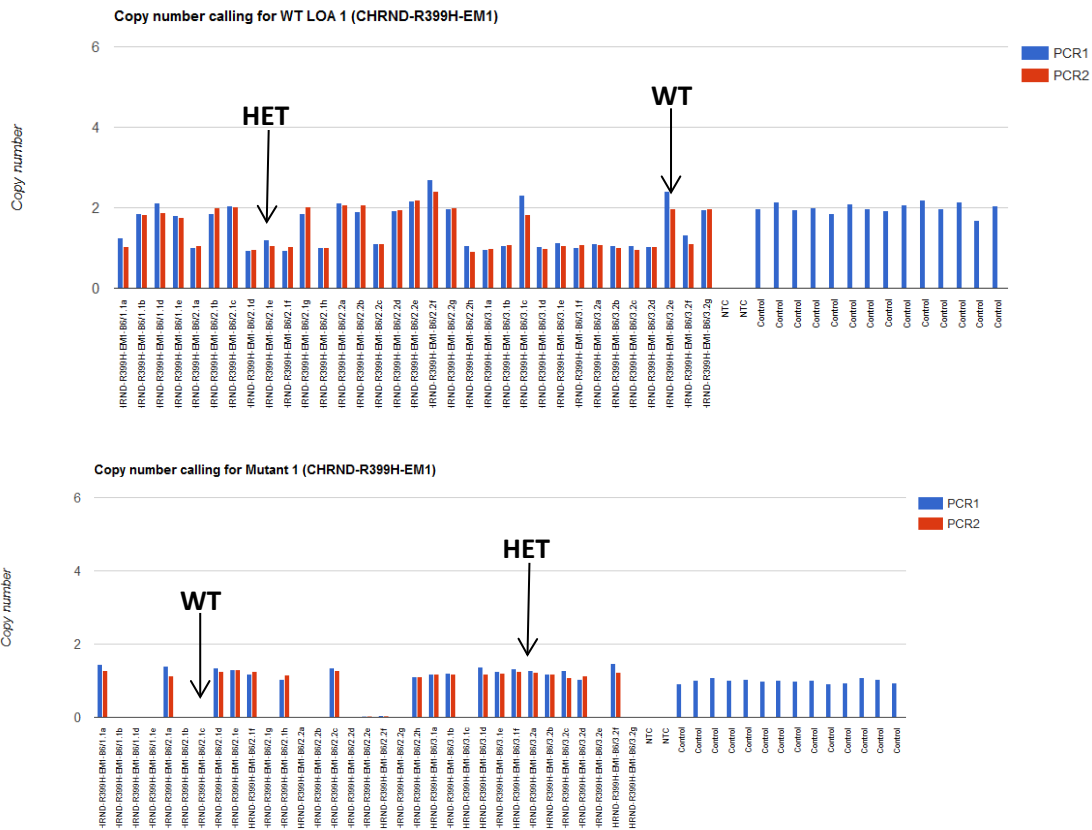

Version No. 1

Date: 28/06/19

Created/Updated by: Daniel Ford

Approved by:

Name of Mouse model or mutation:**Chrnd-R399H-EM1-B6****Description:**

Point mutation generated using CRISPR/Cas9 reagents.

Type of mutation:

Point mutation: R399H


Sequence details**Chrnd WT:**

ATGAGGGACCGTTGAAAGCATTCTACACCAGTCAGTGGGGAGTCTGGGAAACAGACAATGGGGTC
AGCCTGGGAGCTCTATGCGGCAACCAGGGTCCTCAGAATGTGTAAAGATGACTCCACACTTGTGAA
ATGGCCTGTCTTGTGTCCCCCTGACTGCTAAAGTTCTTCTGGAGACCCTGCCAAGCTCCTGCACAT
GTCCCGCCAGCAGAGGAAGACCCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATA
CATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTCCCGCAGTGACCTCATGTTTGAGAAGCAATCA
GAGCGGCATGGGCTGGCCCCGGCGCCTCACCACAGCCCCTGAGTTCTGGTAGCCTTGGAACGTGGCC
CATGTGTGGGAGGTGGGCAATGATAGGCATCATGCCTGCCCTGGCCTCTGTCCACAGGCAGGCCT
CCAGCAAGCTCTGAGCAGGTCCAACAGGAGCTCTTCAATGAGATGAAGCCAGCTGTGGATGGGGCA
AACTTCATCGTCAACCATATGAGAGACAAAACAGTTACAATGAGGTGAGCGACCTGAGACACCAT
AGAATCAGATGTTCAAGTAGACTAGGGATCAAGTGGATTCTGTCTCCCCCTCATAGACACATGTCCA
CTTAGATGAAGAGATGCATGGTGGGTAAGGGACC

Chrnd-R399H-EM1-B6:

ATGAGGGACCGTTGAAAGCATTCTACACCAGTCAGTGGGGAGTCTGGGAAACAGACAATGGGGTC
AGCCTGGGAGCTCTATGCGGCAACCAGGGTCCTCAGAATGTGTAAAGATGACTCCACACTTGTGAA
ATGGCCTGTCTTGTGTCCCCCTGACTGCTAAAGTTCTTCTGGAGACCCTGCCAAGCTCCTGCACAT
GTCCCGCCAGCAGAGGAAGACCCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATA
CATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTCA**ACA**CAGTGACCTCATGTTTGAGAAGCAATCA
GAGCGGCATGGGCTGGCCCCGGCGCCTCACCACAGCCCCTGAGTTCTGGTAGCCTTGGAACGTGGCC
CATGTGTGGGAGGTGGGCAATGATAGGCATCATGCCTGCCCTGGCCTCTGTCCACAGGCAGGCCT
CCAGCAAGCTCTGAGCAGGTCCAACAGGAGCTCTTCAATGAGATGAAGCCAGCTGTGGATGGGGCA
AACTTCATCGTCAACCATATGAGAGACAAAACAGTTACAATGAGGTGAGCGACCTGAGACACCAT
AGAATCAGATGTTCAAGTAGACTAGGGATCAAGTGGATTCTGTCTCCCCCTCATAGACACATGTCCA
CTTAGATGAAGAGATGCATGGTGGGTAAGGGACC

Chrnd-R399H-EM1-B6 Heterozygous F1 animal sequence trace:

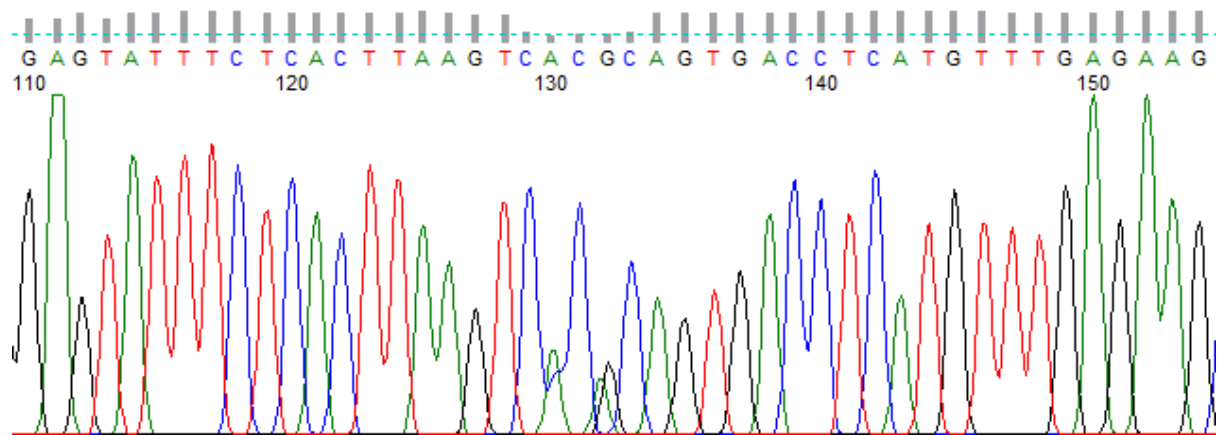

Nucleotide Alignment:

```

|
Chrnd_WT : ATGAGGGACCGTTGAAAGCATTCTACACCAGTCAGTGGGGAGTCTGGGAAACAGACAATGGGGTCAGCCTGGGAGCTCTATGCGGCAACCAGGGTCCTCAGAATGTGTAAGATGACTCCACACTTGTGAAATGGCCGTCTTGTGTCCTCCCTGACTGCTAAAAGTCTTCCT : 172
Chrnd_R399 : ATGAGGGACCGTTGAAAGCATTCTACACCAGTCAGTGGGGAGTCTGGGAAACAGACAATGGGGTCAGCCTGGGAGCTCTATGCGGCAACCAGGGTCCTCAGAATGTGTAAGATGACTCCACACTTGTGAAATGGCCGTCTTGTGTCCTCCCTGACTGCTAAAAGTCTTCCT : 172
          ATGAGGGACCGTTGAAAGCATTCTACACCAGTCAGTGGGGAGTCTGGGAAACAGACAATGGGGTCAGCCTGGGAGCTCTATGCGGCAACCAGGGTCCTCAGAATGTGTAAGATGACTCCACACTTGTGAAATGGCCGTCTTGTGTCCTCCCTGACTGCTAAAAGTCTTCCT

Chrnd_WT : GGAGACCCCTGCCAAGCTCCTGCACATGTCCCGCCAGCAGAGGAAGACCCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATACATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTC C CAGTGACCTCATGTTTGAGAAGCAATCAGAGCGGCATGGG : 344
Chrnd_R399 : GGAGACCCCTGCCAAGCTCCTGCACATGTCCCGCCAGCAGAGGAAGACCCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATACATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTC C CAGTGACCTCATGTTTGAGAAGCAATCAGAGCGGCATGGG : 344
          GGAGACCCCTGCCAAGCTCCTGCACATGTCCCGCCAGCAGAGGAAGACCCAGGCCCCAGGGCTCTCATCCGGAGAAGCAGCTCTCTGGGATACATCTGCAAAGCAGAGGAGTATTTCTCACTTAAGTC C CAGTGACCTCATGTTTGAGAAGCAATCAGAGCGGCATGGG

Chrnd_WT : CTGGCCCGGCGCCTCACCACAGCCGTGAGTTCCTGGTAGCCTTGGAACTGGCCCATGTGTGGGAGGTGGGCAATGATAGGCATCATGCCTGCCCTGGCCTCTGTCCACAGGCAGGCCTCCAGCAAGCTCTGAGCAGGTCCAACAGGAGCTCTTCAATGAGATGAAGCCAG : 516
Chrnd_R399 : CTGGCCCGGCGCCTCACCACAGCCGTGAGTTCCTGGTAGCCTTGGAACTGGCCCATGTGTGGGAGGTGGGCAATGATAGGCATCATGCCTGCCCTGGCCTCTGTCCACAGGCAGGCCTCCAGCAAGCTCTGAGCAGGTCCAACAGGAGCTCTTCAATGAGATGAAGCCAG : 516
          CTGGCCCGGCGCCTCACCACAGCCGTGAGTTCCTGGTAGCCTTGGAACTGGCCCATGTGTGGGAGGTGGGCAATGATAGGCATCATGCCTGCCCTGGCCTCTGTCCACAGGCAGGCCTCCAGCAAGCTCTGAGCAGGTCCAACAGGAGCTCTTCAATGAGATGAAGCCAG

Chrnd_WT : CTGTGGATGGGCAAACCTTCATCGTCAACCATATGAGAGACCAAAACAGTTACAATGAGGTGAGCGACCTGAGACACCATAGAATCAGATGTTCAAGTAGACTAGGGATCAAGTGGATTCTGTCTCCCTCATAGACACATGTCCACTTAGATGAAGAGATGCATGGTGGG : 688
Chrnd_R399 : CTGTGGATGGGCAAACCTTCATCGTCAACCATATGAGAGACCAAAACAGTTACAATGAGGTGAGCGACCTGAGACACCATAGAATCAGATGTTCAAGTAGACTAGGGATCAAGTGGATTCTGTCTCCCTCATAGACACATGTCCACTTAGATGAAGAGATGCATGGTGGG : 688
          CTGTGGATGGGCAAACCTTCATCGTCAACCATATGAGAGACCAAAACAGTTACAATGAGGTGAGCGACCTGAGACACCATAGAATCAGATGTTCAAGTAGACTAGGGATCAAGTGGATTCTGTCTCCCTCATAGACACATGTCCACTTAGATGAAGAGATGCATGGTGGG

Chrnd_WT : TAAGGGACC : 697
Chrnd_R399 : TAAGGGACC : 697
          TAAGGGACC
  
```

Predicted Protein Alignment:

```

*          100
SLGYICKAEEYFSLKS ESDLMFE
SLGYICKAEEYFSLKS ESDLMFE
SLGYICKAEEYFSLKS S DLMFE
  
```


QC strategy employed at Harwell to check the edited allele:

Genomic DNA was extracted from ear clip biopsies and amplified in a PCR reaction using the following conditions/primer sequences:

Geno_CHRND_R399H_F2	ATGAGGGACCGTTGAAAGCA
Geno_CHRND_R399H_R2	GGTCCCTTACCCACCATGC
Taq Polymerase used	Roche Expand Long Range DNTPack
Annealing Temperature (°C)	63
Elongation time (min)	1
WT product size (bp)	697
Mutant product size (bp)	697
Notes	3% DMSO

All amplicons were sent for Sanger sequencing to check for integration of the donor oligo sequence at the target site. F1 sequences should be heterozygous unless on sex chromosome.

Copy counting of the donor sequence was carried out by ddPCR at the F1 stage to confirm donor oligos were inserted once on target into the genome. The following Taqman assay was used to copy count the donor sequence compared against a VIC-labelled reference assay for Dot11:

Assay name	Chrnd-R399H-donor-UNIV1
Forward Primer (5'-3')	GCAGCTCTCTGGGATACATC
Reverse Primer (5'-3')	TGCCGCTCTGATTGCTTCTC
Probe (5'-3')	TGCAAAGCAGAGGAGTATTTCTCACTTA
Label	FAM-BHQ1

The ddPCR assay recognises sequence common to both the WT Chrnd and the R399H mutant. Therefore, WT controls and correctly targeted F1 R399H heterozygote animals will call at 2 copies.

Assay name	Chrnd-R399H-donor-MUT1
Forward Primer (5'-3')	CAGAGGAGTATTTCTCACTTAAGTCACA
Reverse Primer (5'-3')	CGTTCCAAGGCTACCAGAACTC
Probe (5'-3')	CAGTGACCTCATGTTTGAGAAGCAATCA
Label	FAM-BHQ1

The ddPCR assay is specific to the Chrnd R399H mutation. Therefore, WT controls will call at 0 copies and correctly targeted F1 R399H heterozygote animals will call at 1 copy.

Reference Assay Name	Dot1l
Forward primer (5'-3')	GCCCCAGCACGACCATT
Reverse primer (5'-3')	TAGTTGGCATCCTTATGCTTCATC
Probe (5'-3')	CCCAACAGGCCTGGATTCTCAATGC
Label	VIC

VIC-labelled reference assay for Dot1l gene.